

GAFCHROMIC™

DOSIMETRY MEDIA, TYPE EBT-3

WARNING: Store below 25°C
Store away from radiation sources
Do not expose film to sunlight
Handle film carefully, creasing may cause damage
Do not expose to temperatures above 50°C

CONTENTS: 25 sheets, 8" x 10"

GAFCHROMIC™ EBT3 Dosimetry Film

GAFChromic EBT-3 is designed for the measurement of absorbed doses of ionizing radiation. It is particularly suited for high-energy photons. The dynamic range of this film is designed for best performance in the dose range from 0.2 to 10 Gy, making it suitable for many applications in IMRT, VMAT and brachytherapy. For measurement of doses substantially greater than 10 Gy EBT-XD or MD-V3 are preferred while the use of HD-V2 is indicated for still higher dose measurement.

The structure of EBT3 film is shown in Figure 1. The film is comprised of an active layer, nominally 28 µm thick, sandwiched between two 125 µm matte-polyester substrates. The active layer contains the active component, a marker dye, stabilizers and other components giving the film its near energy-independent response. The thickness of the active layer will vary slightly between different production lots. .

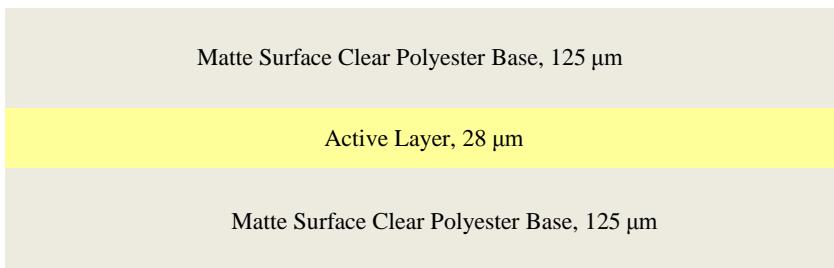


Figure 1: Structure of GAFChromic EBT3 Dosimetry Film

Key technical features of GAFChromic EBT3 include:

- Dynamic dose range: 0.1 Gy to 20 Gy
- Optimum dose range: 0.2 Gy to 10 Gy, best suited for applications such as IMRT and VMAT
- Develops in real time without post-exposure treatment;
- Energy-dependence: minimal response difference from 100keV into the MV range;
- Near tissue equivalent;
- High spatial resolution – can resolve features down to 25µm, or less
- Proprietary new technology incorporating a marker dye in the active layer:
 - Enables non-uniformity correction by using multi-channel dosimetry
 - Decreases UV/visible light sensitivity;
- Stable at temperatures up to 60°C;

The yellow marker dye incorporated in EBT3, in conjunction with an RGB film scanner and FilmQAPro software,¹⁻³ enables the dosimetry process to benefit from the application of triple-channel dosimetry.

To learn more about FilmQAPro software and triple-channel film dosimetry, visit www.FilmQAPro.com.

SPECIFICATIONS

Property	GAFChromic™ EBT3 Film
Configuration	Active layer (28 µm) sandwiched between 125 µm matte-surface polyester substrates
Size	8" x 10", other sizes available upon request
Dynamic Dose Range	0.1 to 20 Gy
Energy dependency	<5% difference in net optical density when exposed at 100 keV and 18 MeV
Dose fractionation response	<5% difference in net optical density for a single 25 Gy dose and five cumulative 5 Gy doses at 30 min. intervals
Dose rate response	<5% difference in net optical density for 10 Gy exposures at rates of 3.4 Gy/min. and 0.034 Gy/min.
Stability in light	<5x10 ⁻³ change in optical density per 1000 lux-day
Stability in dark (pre-exposure stability)	<5x10 ⁻⁴ optical density change/day at 23 °C and <2x10 ⁻⁴ density change/day refrigerated
Uniformity	Better than ±3% in sensitometric response from mean; dose uniformity better than ±2% with FilmQAPro and triple-channel dosimetry

PERFORMANCE DATA AND PRACTICAL USER GUIDELINES

Like all other GAFChromic films, EBT3 dosimetry film can be handled in interior room light for short periods without noticeable effects. However, it is suggested that the film should not be left exposed to room light for hours, but rather should be kept in the dark when not in use. When the active component in EBT3 film is exposed to radiation, it reacts to form a blue colored polymer with absorption maxima at approximately 633 nm.

GAFChromic EBT3 dosimetry film is recommended to be used with a 48-bit (16-bit per channel) flatbed color scanner. The EPSON Expression 11000XL Photo scanner, and the now discontinued model 10000XL Photo scanner are the recommended models. These are color scanners that measure the red, green and blue color components of light transmitted by the film at a color depth of 16 bit per channel. These EPSON scanners are particularly recommended due to their large scanning area.

The typical dose response of EBT3 film on an Epson 10000/11000XL scanner is shown in Figure 2. We recommend to fit the calibration curve to a function having the form

$$d_x(D) = a + b/(D-c)$$

where $d_x(D)$ is the optical density of the film in scanner channel x at dose D, and a, b, c are the equation parameters to be fitted. The advantages of this type of function are:

- They are simple to invert and determine density as a function of dose, or dose as a function of density

- They have rational behavior with respect to the physical reality that the density of the film increases with increasing exposure yet approaches a near constant value at high exposure. Polynomial functions characteristically have no correspondence to physical reality outside the data range over which they are fitted.
- Since these functions have the described rational behavior, fewer calibration points are required saving time and film: A typical case would use 6-8 points (including unexposed film) with the doses in geometric progression.

Detailed instructions defining the optimum procedure for scanning radiochromic film, establishing a calibration curve using FilmQAPro software and obtaining dose measurements from an application film are contained in the document [Efficient Protocols for Calibration and Dosimetry Films](#) on this web site. The procedures described have been thoroughly validated and are in widespread use in the medical physics community providing dose measurement uncertainty well below 2%.

PERFORMANCE COMPARISON BETWEEN GAFCHROMIC EBT3 AND EBT-XD FILMS

As mentioned earlier, GAFChromic EBT3 is specifically designed to obtain optimum results for the applications where the maximum dose is <10 Gy. The high dose associated single or low-fraction applications such as SRS or SBRT poses challenges for the use of EBT3^{5,4}. The two main problems are the increased dose uncertainty at high dose and the impact of the lateral response artifact for wide exposure fields⁶⁻⁹.

Due to the chromatic nature of GAFChromic film, there is no clear color saturation point. This is an advantage when FilmQAPro Pro software is used for the dosimetry analysis, since the use of the three available color channels effectively extends the dynamic range of the film. However, increasingly shallow slopes of the EBT3 response curves at doses >10 Gy may lead to increased dose uncertainty in this high dose region. As seen in Figure 2, EBT-XD film provides steeper slopes of the red and green response functions than EBT3 at higher doses and is therefore more desirable for measurements at doses >10 Gy.,

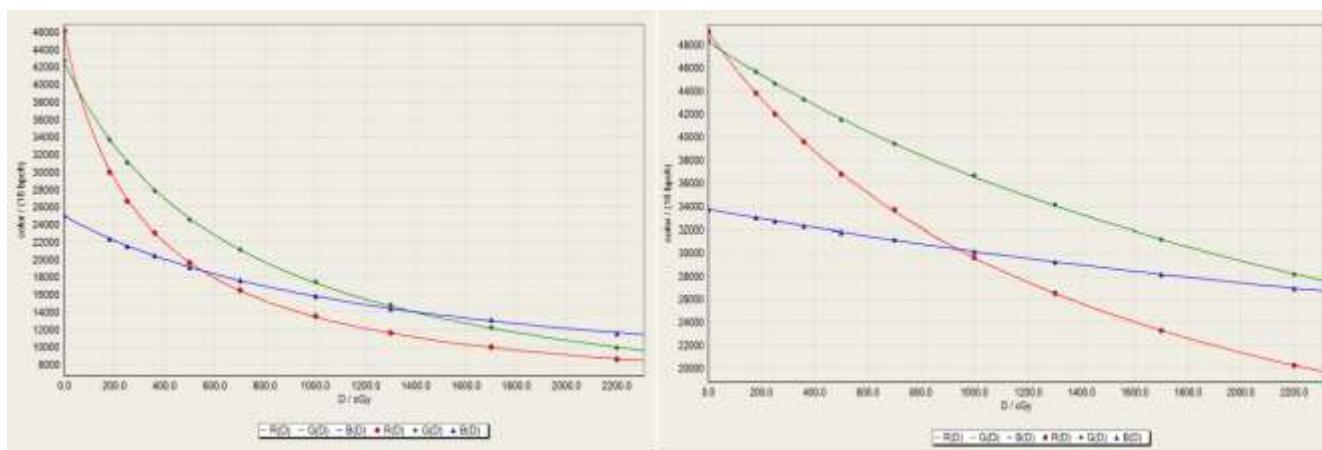


Figure 2. Comparison of Calibration Curves of GAFChromic EBT3 (left) and EBT-XD (right) films

As noted in many publications⁵⁻⁸, flatbed scanners used for radiochromic film measurement

exhibit a lateral scan artifact (LRA), i.e., the color value measured varies depending upon the location of the film placement relative to the center of the scanner. Typically, film scanned away from the center location appears to have greater optical density resulting in a higher calculated dose. The deviation also increases with increasing dose.

The LRA occurs for two reasons. The major cause is the polarization of light transmitted by the film and its subsequent interaction with the mirrors in the optical train of the scanner. Upon exposure, the active component in the film polymerizes to form a colored polymer that polarizes transmitted light¹⁰. On a flatbed scanner the polarized transmitted light is guided to the CCD detector by a series of mirrors and a lens. At the lateral center of the scan area rays are incident normal to the plane of the mirrors, but the angle of incidence increases as the distance from the center increases. As the rays transmitted by the film pass through the optical system the reflectivity of the mirrors is influenced by the angle of incidence of the polarized light. As a consequence, for films with the same transmission placed at the lateral center and side of the scanner, the detected signal will be greater at the center and diminish towards the side of the scanner. A smaller effect, due to the geometry of the optical system in flatbed scanners, results in an increase in the path-length of light through the film towards the lateral edges of the scanner. By the Beer-Lambert Law, this causes transmission to decrease with increasing distance from the center of the scanner, reinforcing the effects caused by polarization⁹.

REFERENCES

1. Micke, A., Lewis, D.F., Yu, X. "Multichannel film dosimetry with non-uniformity correction," *Med Phys*, 38(5), 2523-2534 (2011).
2. Lewis D., Micke A., Yu X, Chan M.: "An Efficient Protocol for Radiochromic Film Dosimetry combining Calibration and Measurement in a Single Scan", *Medical Physics*, 39 (10) 6339(2012)
3. An Efficient Calibration Protocol for Radiochromic Film, April 2011 available at www.filmqapro.com
4. **GAFChromic™ EBT3 film specifications**, Available at www.gafchromic.com
5. Mathot M, et al., "GAFChromic film dosimetry: Four years' experience using FilmQA Pro software and Epson flatbed scanners", *Physica Medica* (2014)
6. Schoenfeld A, et al, "The artefacts of radiochromic film dosimetry with flatbed scanners and their causation by light scattering from radiation-induced polymers", *Phys. Med. Biol.* 59 (2014) 3575
7. D. Lewis and M F. Chan, "Correcting lateral response artifacts from flatbed scanners for radiochromic film dosimetry", *Med. Phys.* 42, 416-429 (2015)
8. L. J. van Battum, H. Huizenga, R. M. Verdaasdonk and S. Heukelom,, "How flatbed scanners upset accurate film dosimetry", *Physics in Medicine and Biology*, 61(2016), 625-649
9. B. Reimer and H. Baessler, "Photoconduction in a Polydiacetylene Crystal", *Physica Status Solidi* 32(2), 435–439 (1975)